
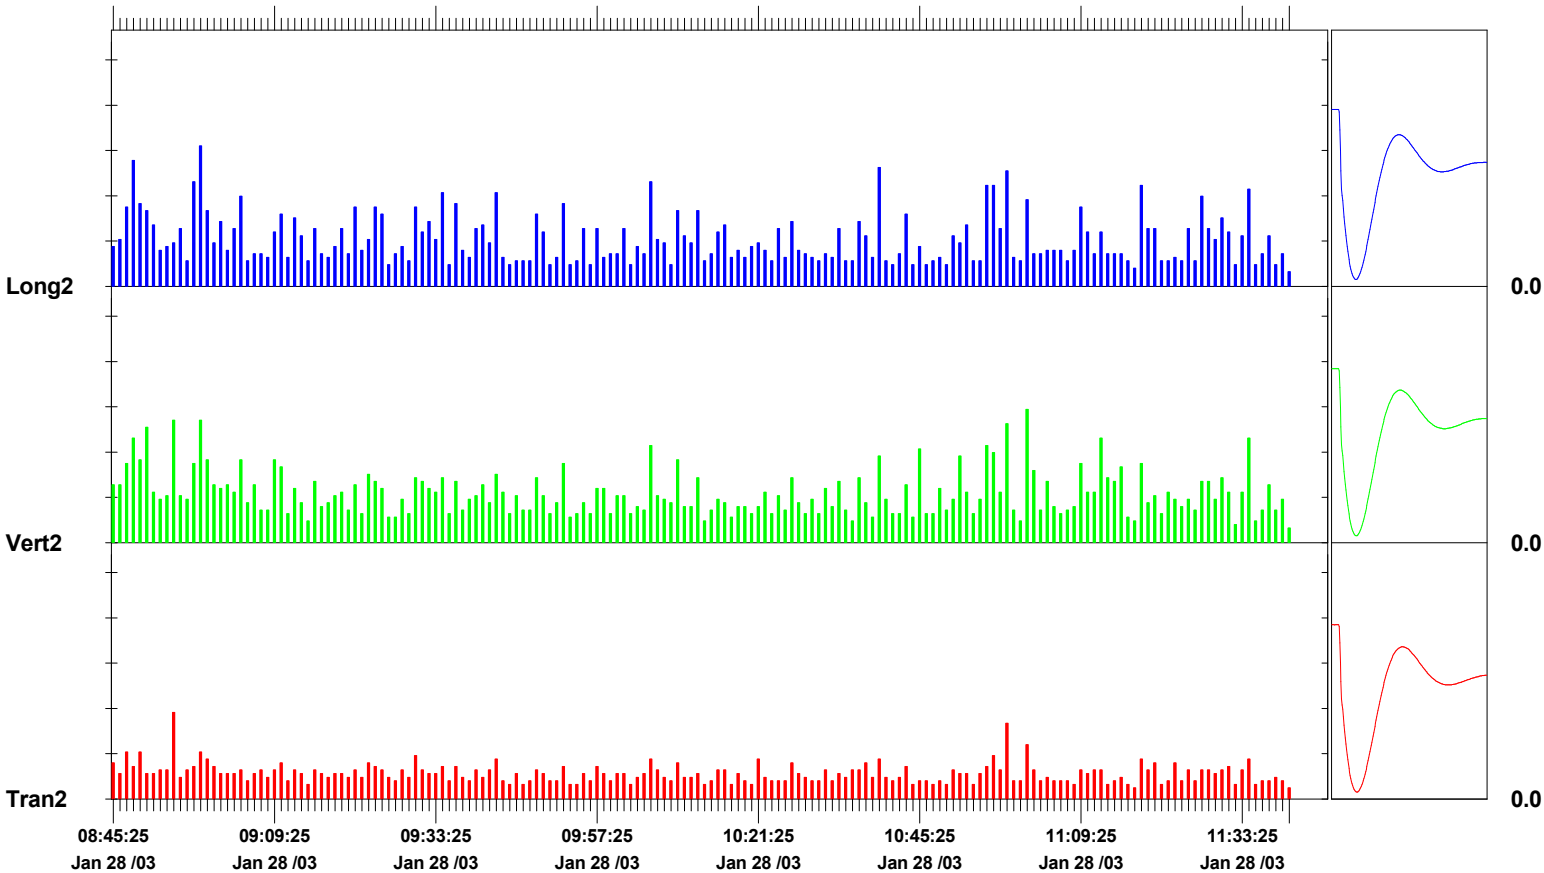


Histogram Start Time 08:44:25 January 28, 2003
Histogram Finish Time 11:39:58 January 28, 2003
Number of Intervals 5266.00 at 2 seconds
Range Geo:31.75 mm/s
Sample Rate 1024sps
Job Number: 2122

Serial Number BE6178 V 7.0-4.35 MiniMate Plus/8
Battery Level 6.1 Volts
Unit Calibration January 10, 2003 by InstanTel Inc.
File Name I0358WST.M10

	Tran2	Vert2	Long2	
PPV	0.381	0.587	0.619	mm/s
ZC Freq	64	12	11	Hz
Date	Jan 28 /03	Jan 28 /03	Jan 28 /03	
Time	08:53:59	11:01:17	08:57:53	
Sensor Check	Passed	Passed	Passed	
Frequency	7.0	7.3	7.4	Hz
Overswing Ratio	3.9	3.8	3.9	
Peak Vector Sum	379.3 mm/s on January 28, 2003 at 11:39:58			

USBM RI8507 And OSMRE

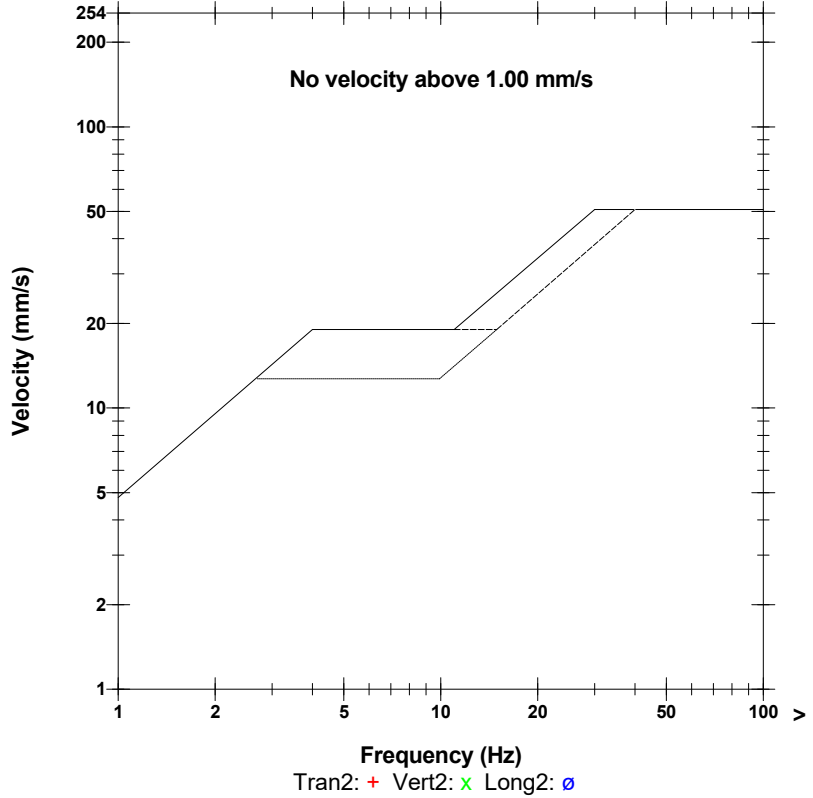

Time Scale: 1 minute /div Amplitude Scale: Geo: 0.200 mm/s/div

Sensor Check